


# Nanospray of Combichem Compounds in pure DMSO

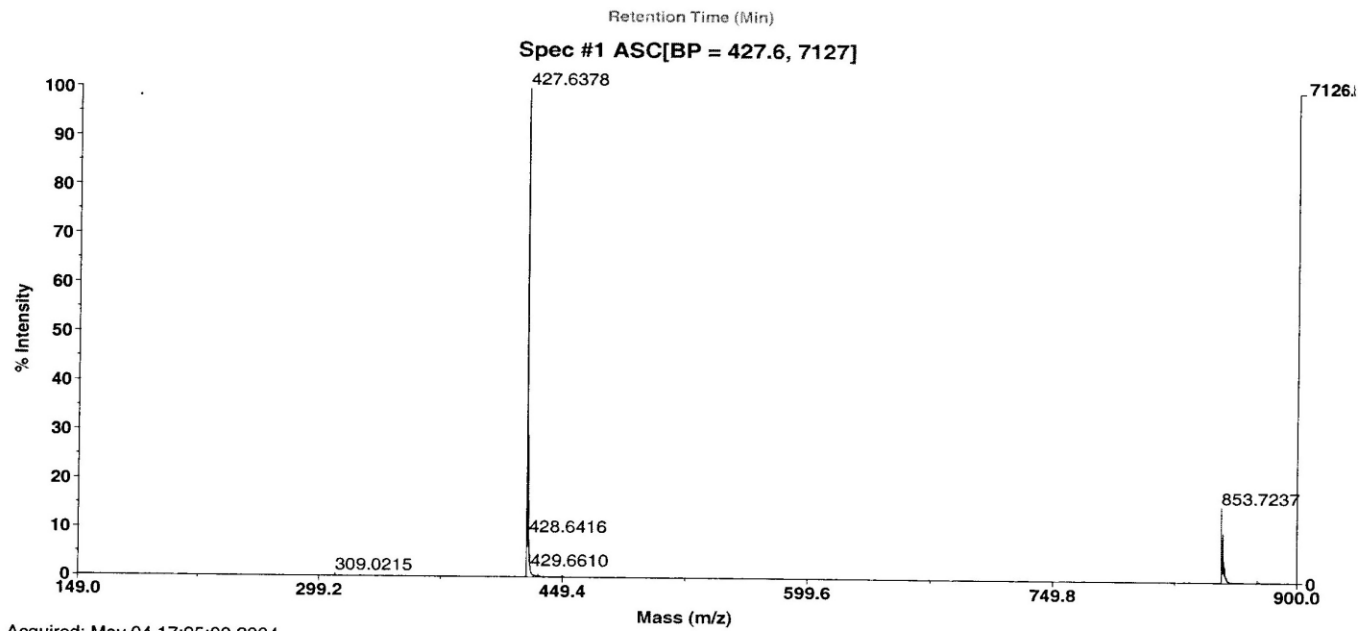

2  $\mu$ L drop of combichem compound without diluting or washing off the DMSO. Since the concentration was high (mg/mL), the nozzle was placed  $\sim$  5 cm from the mass spectrometer inlet. The mass spectrometer used was a Mariner TOF.